

Alcotest 7110 Calibration Record


Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0056
Location:	LONG BRANCH POLICE DEPT	
Calibration File No.:	00779	Calib. Date: 05/30/2019
Certification File No.:	00747	Cert. Date: 12/13/2018
Linearity File No.:	00748	Lin. Date: 12/13/2018
Solution File No.:	00778	Soln. Date: 05/27/2019
Sequential File No.:	00779	File Date: 05/30/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXN S3-0217
Solution Control Lot:	18220	Expires: 07/23/2020
		Bottle No.: 0649

Coordinator

Last Name: LUTZ	First Name: DENNIS	MI: J
Signature: <u>Tpr I Dennis 7045</u>		
	Badge No.: 7045	
	Date: 05/30/2019	

*Black Key Temperature Probe Serial.....# DDEEP2-060 (LC)

*Digital NIST Temperature Measuring System Serial.....# 191 959 024 (LC)

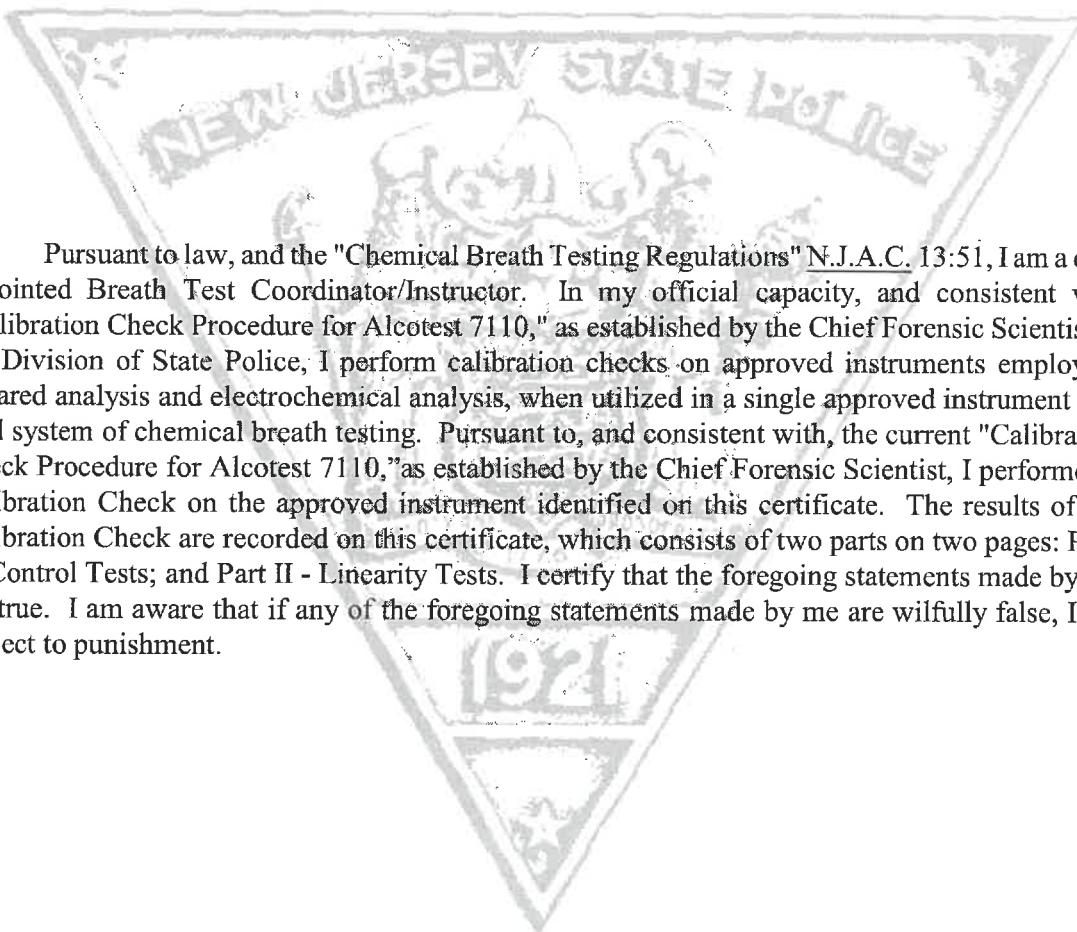Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0056
Location:	LONG BRANCH POLICE DEPT	
Calibration File No.:	00779	Calib. Date: 05/30/2019
Certification File No.:	00780	Cert. Date: 05/30/2019
Linearity File No.:	00748	Lin. Date: 12/13/2018
Solution File No.:	00778	Soln. Date: 05/27/2019
Sequential File No.:	00780	File Date: 05/30/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXN S3-0217
Solution Control Lot:	18220	Expires: 07/23/2020
		Bottle No.: 0649

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:14D		
Control 1 EC	0.099%	12:15D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:15D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:16D		
Control 2 EC	0.098%	12:17D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:17D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:17D		
Control 3 EC	0.097%	12:18D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	12:18D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:19D		

All tests within acceptable tolerance.

Coordinator

Last Name: LUTZ

Signature: Tpr I Dennis

First Name: DENNIS

MI: J

Badge No.: 7045

Date: 05/30/2019

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests


Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0056		
Location:	LONG BRANCH POLICE DEPT			
Calibration File No.:	00779	Calib. Date: 05/30/2019		
Certification File No.:	00780	Cert. Date: 05/30/2019		
Linearity File No.:	00781	Lin. Date: 05/30/2019		
Solution File No.:	00778	Soln. Date: 05/27/2019		
Sequential File No.:	00781	File Date: 05/30/2019		
Calibrating Unit:	WET	Model No.: CU-34		
Control Solution %:	0.040%	Serial No.: DDSC S3-0001		
Solution Control Lot:	17240	Expires: 08/10/2019 Bottle No.: 1164		
Calibrating Unit:	WET	Model No.: CU-34		
Control Solution %:	0.080%	Serial No.: DDXC S3-0020		
Solution Control Lot:	18250	Expires: 08/06/2020 Bottle No.: 1375		
Calibrating Unit:	WET	Model No.: CU-34		
Control Solution %:	0.160%	Serial No.: DDMK S3-0008		
Solution Control Lot:	17260	Expires: 08/21/2019 Bottle No.: 0609		
Function	Result	Time	Temperature	Comment(s)
Ambient Air Blank	0.000%	12:27D	Simulator (°C)	or Error(s)
Control 1 EC	0.041%	12:28D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.037%	12:28D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:30D		
Control 2 EC	0.040%	12:30D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.040%	12:30D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:32D		
Control 3 EC	0.081%	12:33D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.078%	12:33D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:34D		
Control 4 EC	0.078%	12:35D	33.9°C	*** TEST PASSED ***
Control 4 IR	0.078%	12:35D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:37D		
Control 5 EC	0.159%	12:38D	33.9°C	*** TEST PASSED ***
Control 5 IR	0.156%	12:38D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:39D		
Control 6 EC	0.157%	12:40D	33.9°C	*** TEST PASSED ***
Control 6 IR	0.155%	12:40D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:42D		

All tests within acceptable tolerance.

Coordinator

Last Name: LUTZ

Signature: _____

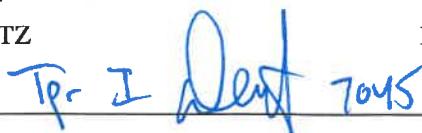

First Name: DENNIS

MI: J

Badge No.: 7045

Date: 05/30/2019

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0056		
Location:	LONG BRANCH POLICE DEPT			
Calibration File No.:	00779	Calib. Date: 05/30/2019		
Certification File No.:	00780	Cert. Date: 05/30/2019		
Linearity File No.:	00781	Lin. Date: 05/30/2019		
Solution File No.:	00782	Soln. Date: 05/30/2019		
Sequential File No.:	00782	File Date: 05/30/2019		
Calibrating Unit:	WET	Model No.: CU-34		
Control Solution %:	0.100%	Serial No.: DDXN S3-0217		
Solution Control Lot:	19060	Expires: 02/11/2021		
		Bottle No.: 0686		
Function	Result	Time	Temperature	Comment(s) or Error(s)
Ambient Air Blank	0.000%	HH:MM 14:53D	Simulator (°C)	
Control 1 EC	0.100%	14:54D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:54D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:55D		
Control 2 EC	0.099%	14:56D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	14:56D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:57D		
Control 3 EC	0.098%	14:58D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	14:58D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:59D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with
Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number:

DDEEP2-096

(DL)

Changed By:

Last Name: LUTZ

First Name: DENNIS

MI: J

Signature:

Tpr I Det 7045

Badge No.: 7045

Date: 05/30/2019

**Alcotest 7110 MKIII-C Calibration
NIST-Traceable Digital Thermometer Readings**

Coordinator:

Tpr I Dennis J Lutz
Name

7045
Badge No.

Location:

Long Branch Police Dept
Agency

ARXA-0056

Alcotest Serial No.

Equipment:

191 959 024
Digital NIST Temperature Measuring System Serial No.

Simulator Solution Concentration	CU-34 Simulator Serial No.	Time Simulators Started to Heat	Time Temp. Reading Obtained	Temp. Reading on NIST Traceable Thermometer
0.04%	DDSC S3-0001	11:04 D	12:06 D	34.0 °C
0.08%	DDXC S3-0020	11:04 D	12:06 D	33.9 °C
0.10%	DDXN S3-0217	11:04 D	12:07 D	34.0 °C
0.16%	DDMK S3-0008	11:04 D	12:08 D	34.0 °C

Pursuant to law and the "Chemical Breath Testing Regulations" established at N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity and consistent with the "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on Alcotest 7110 MKIII-C instruments. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110", I performed a Calibration Check Procedure on the Alcotest 7110 MKIII-C instrument identified on this certificate. Pursuant to the current "Calibration Check Procedure for Alcotest 7110", I used the Digital NIST-traceable Temperature Measuring System identified on this certificate to confirm that the temperatures of the 0.10%, 0.04%, 0.08%, and 0.16% Simulator Solutions used in the respective CU-34 Simulators identified on this certificate, were 34.0 degrees Celsius \pm 0.2 degrees Celsius. I hereby certify that I truthfully recorded on this certificate the temperatures of each of the simulator solutions as shown on the Digital NIST-traceable Temperature Measuring System thermometer. I am aware that if any of the foregoing statements made by me are willfully false, I am subject to punishment.

Tpr I Lutz
Coordinator's Signature

5-30-19
Date



Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

Model: ALCOTEST CU34
 Model: MARK IIA
 Other: _____

Serial Number:

DDSCS3-0001

Certification Date:

1-16-19

Technician:

BS

Re-Certification Due Date:

1-16-20

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

Model: ALCOTEST CU34
 Model: MARK IIA
 Other: _____

Serial Number:

DDXCS3-0020

Certification Date:

1-16-19

Technician:

BS

Re-Certification Due Date:

1-16-20



Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger, Inc.

Model: ALCOTEST CU34
 Model: MARK IIA
 Other: _____

Serial Number:

DDmKS3-0008

Certification Date:

1-16-19

Technician:

BS

Re-Certification Due Date:

1-16-20

Alcotest 7110 Temperature Probe CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDEEP2-000

Certification Date:

7-12-18

Next Certification Due:

7-12-19

Probe Value:

104

Draeger, Inc.

BS



Calibration complies with ISO/IEC 17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-10177843

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International LLC Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA, 19087

Instrument Identification:

Model: 61220-601,

S/N: 191959024

Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath	93139		
Thermistor Module	A17118	20 Apr 2019	1000424560
Thermistor Module	A27129	10 Jan 2020	1000436202
Temperature Calibration Bath	A73332		
Temperature Probe	3039	08 May 2019	6-B7F4L-20-1
Temperature Calibration Bath	A79341		
Temperature Probe	5394	29 Jan 2020	B9124038
Temperature Calibration Bath	B16388		
Temperature Probe	5267	28 Jan 2020	B9124036

Certificate Information:

Technician: 104

Procedure: CAL-06

Cal Date: 13 Feb 2019

Cal Due Date: 13 Feb 2021

Test Conditions: 38.85%RH 24.21°C 1023mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C	N.A.	N.A.		-0.002	-0.002	Y	-0.052	0.048	0.0087	>4:1
°C	N.A.	N.A.		24.999	25.001	Y	24.949	25.049	0.0087	>4:1
°C	N.A.	N.A.		50.001	50.001	Y	49.951	50.051	0.0087	>4:1
°C	N.A.	N.A.		100.003	99.999	Y	99.953	100.053	0.0087	>4:1

This certificate indicates Traceability to standards provided by (NIST) National Institute of Standards and Technology and/or a National Standards Laboratory.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor $k=2$ to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=+(Max-Min)/2; Min=As Left Nominal(Rounded)-Tolerance; Max= As Left Nominal(Rounded) + Tolerance;

Nicol Rodriguez, Quality Manager

Aaron Judge, Technical Manager

Note:

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometer change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.control3.com

Control Company is an ISO/IEC 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2008 Quality Certified by DNV GL, Certificate No. CERT-07805-2006-AQ-HOU-RvA.
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-10177843

Traceable® Certificate of Calibration for Digital Thermometer

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.control3.com

Control Company is an ISO/IEC 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2008 Quality Certified by DNV GL, Certificate No. CERT-01805-2006 AQ-HOU-RVA.
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
Post Office Box 7068
West Trenton, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS 0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 07/31/2018

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 18220

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1210 to 0.1233 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 23, 2020.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Ali M. Alaouie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 1st day of August, 2018.
Mary E. McLaughlin
Notary

MARY ELIZABETH MC LAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PIRRINO
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS 0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 08/29/2017

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 17240

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0483 to 0.0489 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 10, 2019.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaouie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 30th day of August, 2017.

Mary E. McLaughlin
Notary

MARY ELIZABETH MC LAUGHLIN

ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

*New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable*





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS 0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 08/30/2018

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 18250

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0976 to 0.0987 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 06, 2020.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 4th day of September, 2018.

Mary E. McLaughlin
Notary

MARY ELIZABETH MC LAUGHLIN

ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018.



"An Internationally Accredited Agency"

*New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable*





State of New Jersey

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRISTOPHER S. Porrino
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS 0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 09/12/2017

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 17260

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1937 to 0.1957 grams per 100 milliliters of solution.


This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 21, 2019.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Aliaouie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 13 day of September, 2017.

Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
Post Office Box 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS 0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding; the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 02/28/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19060


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1216 to 0.1228 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is February 11, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 6th day of March, 2019.

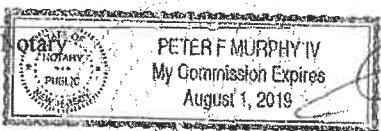

"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



DEPARTMENT OF
Law and Public Safety
This is to certify that

Dennis J. Lutz

Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 7110 MKIII-C

A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 29th DAY OF January

TWO THOUSAND AND Nineteen

Dennis J. Lutz
COLONEL
NEW JERSEY STATE POLICE

ESQ
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES _____

DATE	Refresher Course	PLACE	INSTRUCTOR
1. _____	_____	_____	_____
2. _____	_____	_____	_____
3. _____	_____	_____	_____
4. _____	_____	_____	_____
5. _____	_____	_____	_____
6. _____	_____	_____	_____
7. _____	_____	_____	_____
8. _____	_____	_____	_____
9. _____	_____	_____	_____

S.P. 293B (Rev. 01/18)

DEPARTMENT OF
Law and Public Safety
This is to certify that

Dennis J. Lutz

New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 7110 MKIII-C

A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 1st DAY OF October

TWO THOUSAND AND Nine

Jerry L. Black
SUPERINTENDENT
NEW JERSEY STATE POLICE

One M. Wilson
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES _____

DATE	Refresher Course	PLACE	INSTRUCTOR
1. <u>2-7-11</u>	<u>OCPA</u>	<u>OCPA</u>	<u>Wm. Ross</u>
2. <u>1/14/13</u>	<u>OCPA</u>	<u>OCPA</u>	<u>Adam Steele</u>
3. <u>11-23-15</u>	<u>GCPA</u>	<u>GCPA</u>	<u>M. Goncalves</u>
4. <u>4/6/17</u>	<u>LAKESHORE</u>	<u>LAKESHORE</u>	<u>Adam Steele</u>
5. _____	_____	_____	_____
6. _____	_____	_____	_____
7. _____	_____	_____	_____
8. _____	_____	_____	_____
9. _____	_____	_____	_____

S.P. 293B (Rev. 07/07)

Dräger

Alcotest® 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for breath alcohol measurement device. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EEMT with 49 CFR 4500.4, 49 CFR 4500.5 and 49 CFR 4500.6. The manufacturer recommends accuracy validation of this instrument within 12 months of the calibration date below, or sooner, according to your state specifications.

Calibration Date:

4-15-16 SERIAL NUMBER:
ARXA-0036

Dräger Safety Diagnostics, Inc.



Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

Model: ALCOTEST CU34
 Model: MARK IIA
 X-Cal 2000 (Alcosim)
 Other: _____

Serial Number:

DDXN S3-0217

Certification Date:

4-26-19

Technician:

BS

Re-Certification Due Date:

4-26-20



Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe: Certification Date: Next Certification Due:

DDDEP2-090

4-25-19

4-25-20

Probe Value:

101

Draeger, Inc.

BS