

Alcotest 7110 Calibration Record

Equipment

Alcotest 7110 MKIII-C
Serial No.: ARXA-0056
Location: LONG BRANCH POLICE DEPT
Calibration File No.: 00713
Calib. Date: 07/17/2018
Calib. No.: 00028
Certification File No.: 00683
Cert. Date: 09/14/2017
Cert. No.: 00021
Linearity File No.: 00684
Lin. Date: 09/14/2017
Lin. No.: 00021
Solution File No.: 00710
Soln. Date: 01/26/2018
Soln. No.: 00147
Sequential File No.: 00713
File Date: 07/17/2018


Calibrating Unit: WET
Model No.: CU-34
Serial No.: DDXN S3-0217
Control Solution %: 0.100%
Expires: 08/07/2019
Solution Control Lot: 17230
Bottle No.: 1022

Coordinator

Last Name: PAVLOSKY
First Name: ALLISON
MI: M.
Badge No.: 7330
Date: 07/17/2018

Signature: 

*Black Key Temperature Probe Serial.....# DDXK P2 - 398 A
*Digital NIST Temperature Measuring System Serial.....# 170428364 A

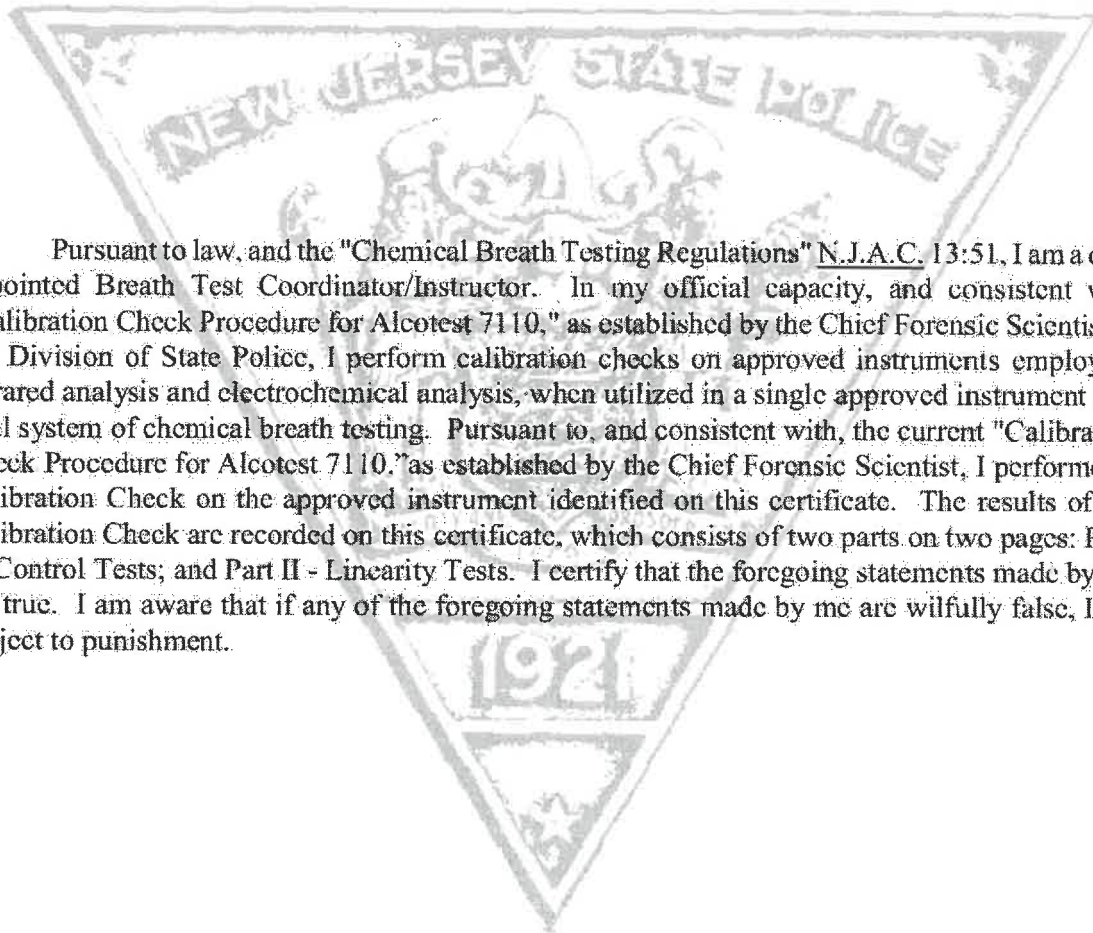

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0056
Location: LONG BRANCH POLICE DEPT
Calibration File No.: 00713 Calib. Date: 07/17/2018 Calib. No.: 00028
Certification File No.: 00714 Cert. Date: 07/17/2018 Cert. No.: 00022
Linearity File No.: 00684 Lin. Date: 09/14/2017 Lin. No.: 00021
Solution File No.: 00710 Soln. Date: 01/26/2018 Soln. No.: 00147
Sequential File No.: 00714 File Date: 07/17/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXN S3-0217
Control Solution %: 0.100% Expires: 08/07/2019
Solution Control Lot: 17230 Bottle No.: 1022

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:36D		
Control 1 EC	0.099%	07:36D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	07:36D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:37D		
Control 2 EC	0.100%	07:38D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	07:38D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:38D		
Control 3 EC	0.100%	07:39D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	07:39D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:40D		

All tests within acceptable tolerance.

Coordinator

Last Name: PAVLOSKY

First Name: ALLISON

MI: M.

Badge No.: 7330

Date: 07/17/2018

Signature: _____

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0056
Location: LONG BRANCH POLICE DEPT
Calibration File No.: 00713 Calib. Date: 07/17/2018 Calib. No.: 00028
Certification File No.: 00714 Cert. Date: 07/17/2018 Cert. No.: 00022
Linearity File No.: 00715 Lin. Date: 07/17/2018 Lin. No.: 00022
Solution File No.: 00710 Soln. Date: 01/26/2018 Soln. No.: 00147
Sequential File No.: 00715 File Date: 07/17/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRK S3-0012
Control Solution %: 0.040% Expires: 08/10/2019
Solution Control Lot: 17240 Bottle No.: 0464

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRK S3-0015
Control Solution %: 0.080% Expires: 08/15/2019
Solution Control Lot: 17250 Bottle No.: 0729

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRK S3-0025
Control Solution %: 0.160% Expires: 08/21/2019
Solution Control Lot: 17260 Bottle No.: 1094

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	07:51D		
Control 1 EC	0.040%	07:52D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.040%	07:52D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:54D		
Control 2 EC	0.040%	07:54D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.040%	07:54D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:56D		
Control 3 EC	0.079%	07:56D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.079%	07:56D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:58D		
Control 4 EC	0.080%	07:59D	33.9°C	*** TEST PASSED ***
Control 4 IR	0.080%	07:59D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:00D		
Control 5 EC	0.160%	08:01D	33.9°C	*** TEST PASSED ***
Control 5 IR	0.160%	08:01D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:02D		
Control 6 EC	0.160%	08:03D	33.9°C	*** TEST PASSED ***
Control 6 IR	0.160%	08:03D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:05D		

All tests within acceptable tolerance.

Coordinator

Last Name: PAVLOSKY

First Name: ALLISON

MI: M.

Signature: _____



Badge No.: 7330

Date: 07/17/2018