

Alcotest 7110 Calibration Record

Equipment

Alcotest 7110 MKIII-C
Serial No.: ARXA-0056
Location: LONG BRANCH POLICE DEPT
Calibration File No.: 00830 Calib. Date: 02/18/2020 Calib. No.: 00032
Certification File No.: 00803 Cert. Date: 09/24/2019 Cert. No.: 00025
Linearity File No.: 00804 Lin. Date: 09/24/2019 Lin. No.: 00025
Solution File No.: 00827 Soln. Date: 01/25/2020 Soln. No.: 00170
Sequential File No.: 00830 File Date: 02/18/2020


Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXN S3-0216
Control Solution %: 0.100% Expires: 07/23/2020
Solution Control Lot: 18220 Bottle No.: 0395

Coordinator

Last Name: LUTZ First Name: DENNIS MI: J
Signature: *Per I Lutz 7045* Badge No.: 7045
Date: 02/18/2020

*Black Key Temperature Probe Serial.....# DDEF, P2-060 DL

*Digital NIST Temperature Measuring System Serial.....# 191 959 029 DL

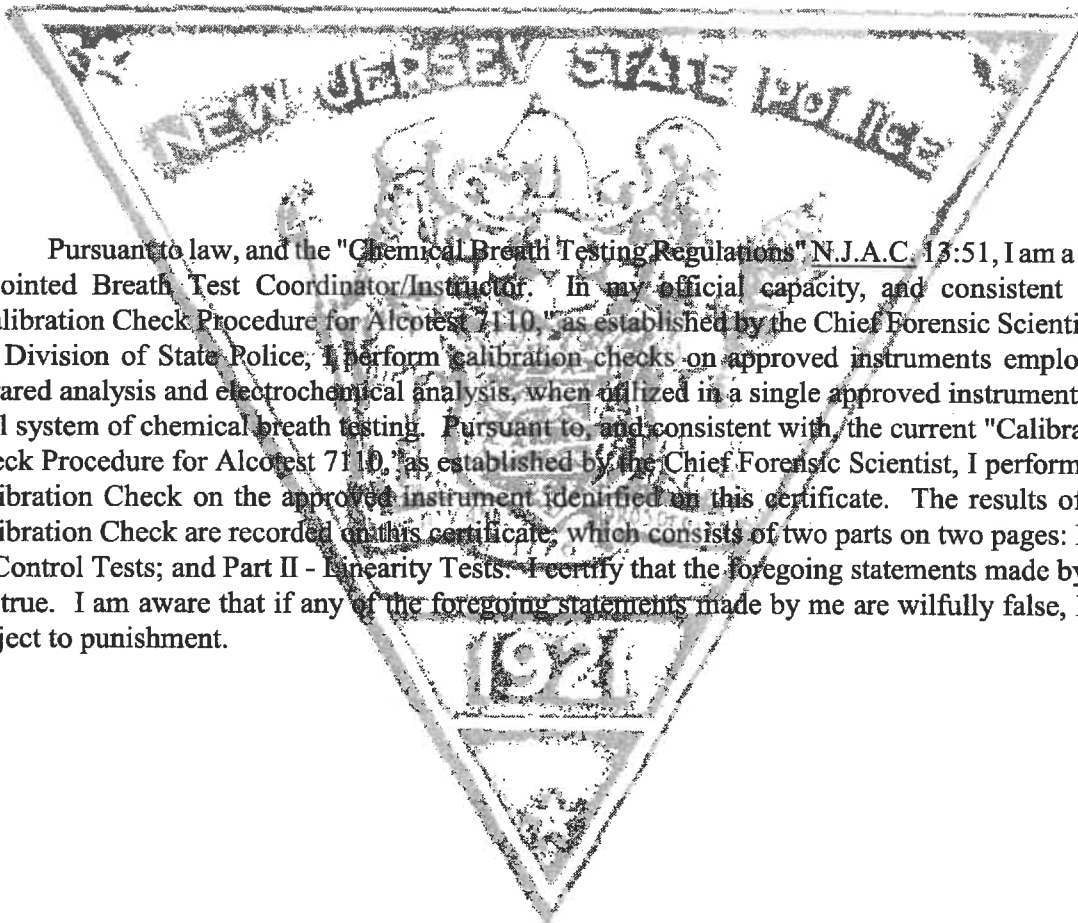

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.